


MICROFILMED

MAG A35

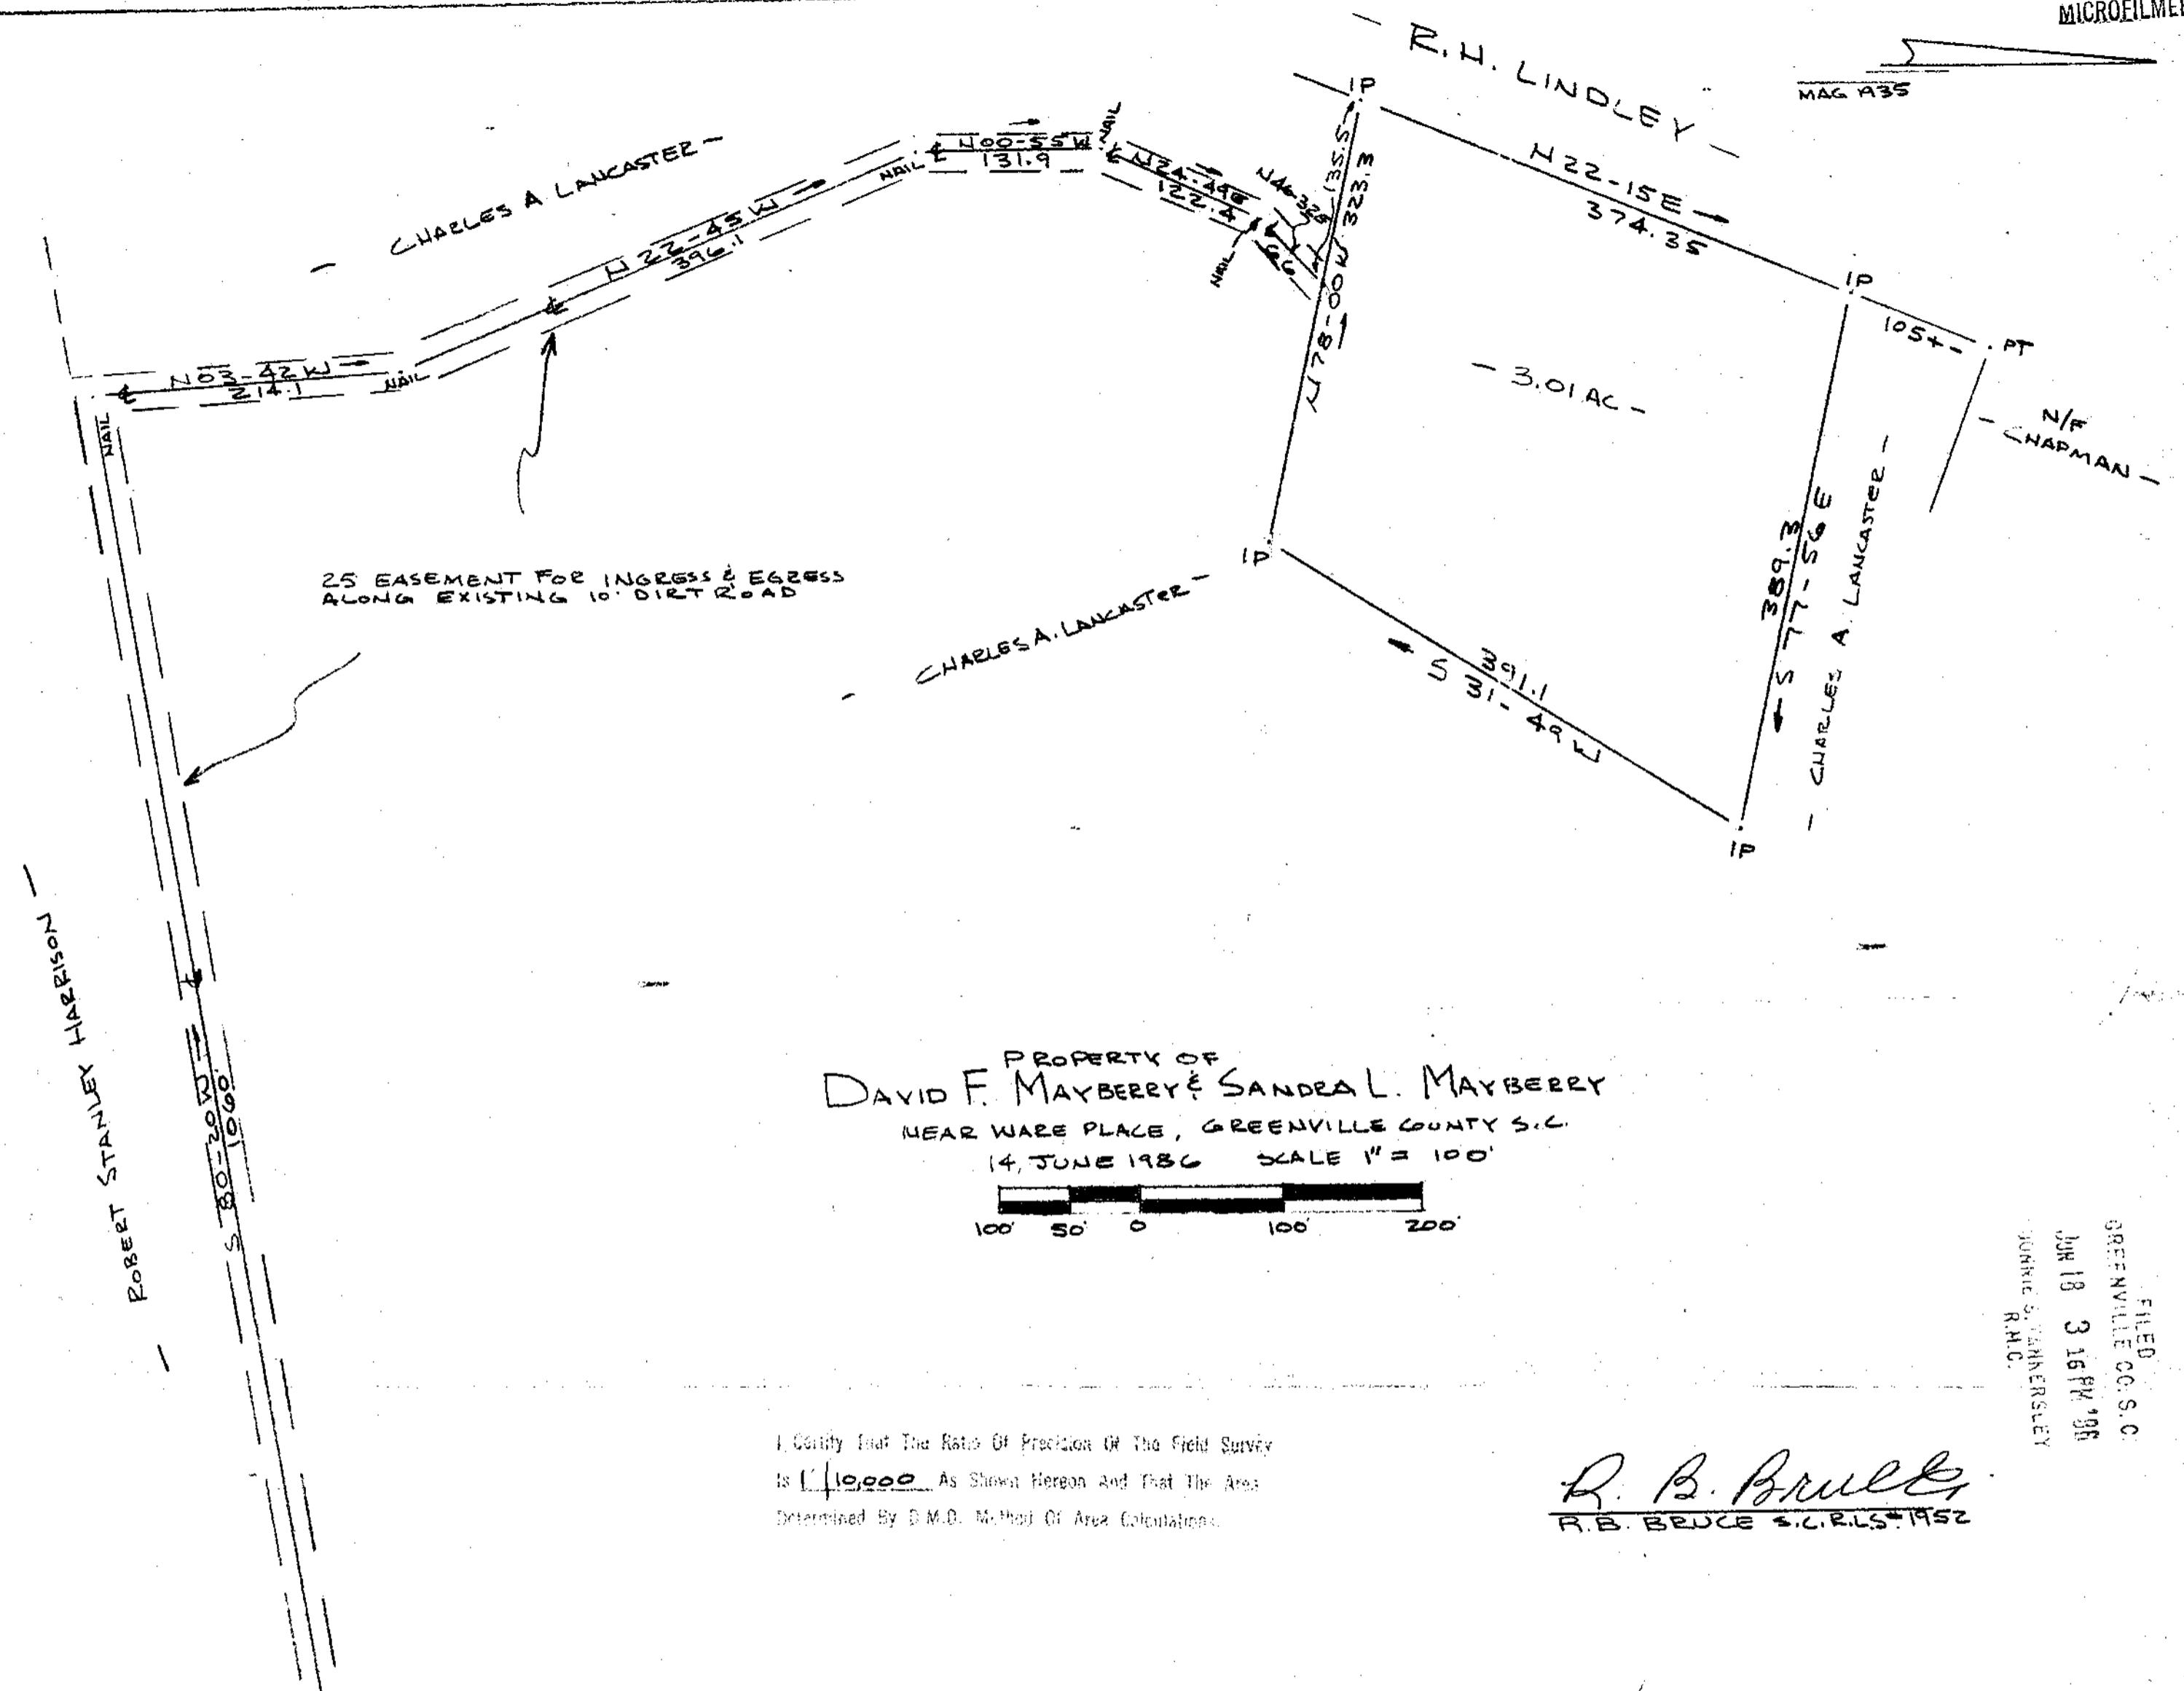


I Certify That The Ratio Of Precision Of The Field Survey
Is 1:10,000 As Shown Heron And That The Areas
Determined By D.M.D. Method Of Area Calculations.

R. B. BRUCE S.C.R.L.S-1952

GREENVILLE CO. S.C.
JULY 18 3 16 PM '96
JUNIOR S. HANBERSLEY
R.H.C.

BELTON ST. NW.Y.
S.C. HWY # 247
(Cooley Bridge Road)

12 u. 50

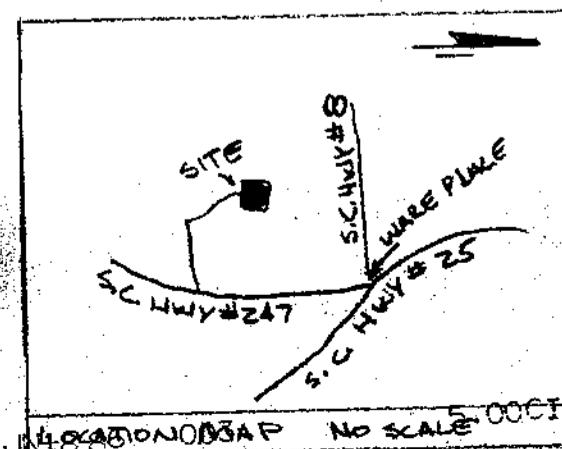

CAROLINA SURVEYING COMPANY
112 MAIN ST. GREENVILLE S.C.

604.1-1-PTZI